


► This document is designed as a reference to be used alongside the Xprecia Stride™ Coagulation Analyzer. For complete instructions, see the *Xprecia Stride User Guide* and the instructions for use that came with your test strips and controls.


PACKAGE CONTENTS

- 1 Xprecia Stride
- 2 Protective Caps (3)
- 3 USB Cable
- 4 AA Batteries (3)

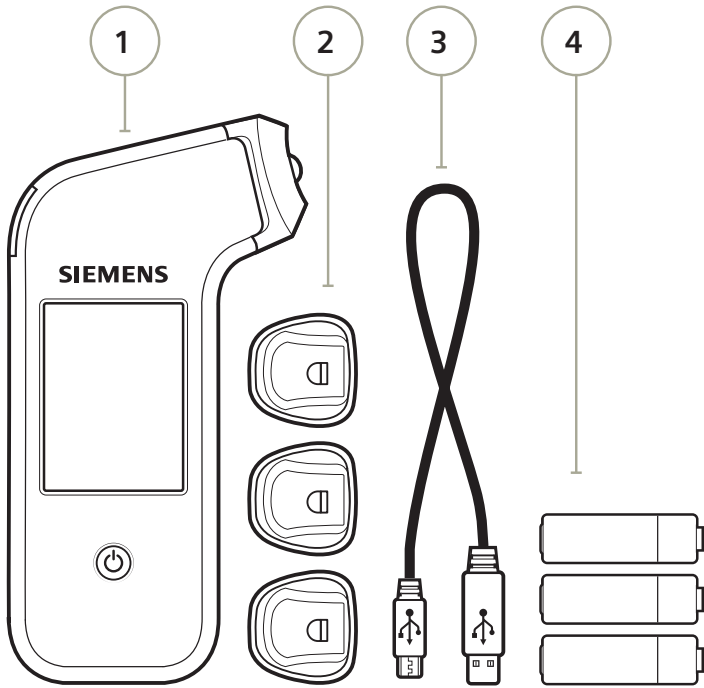


CONSUMABLES

- 1 PT/INR Test Strips
- 2 PT Control 1
- 3 PT Control 2
- 4 CaCl₂ Diluent

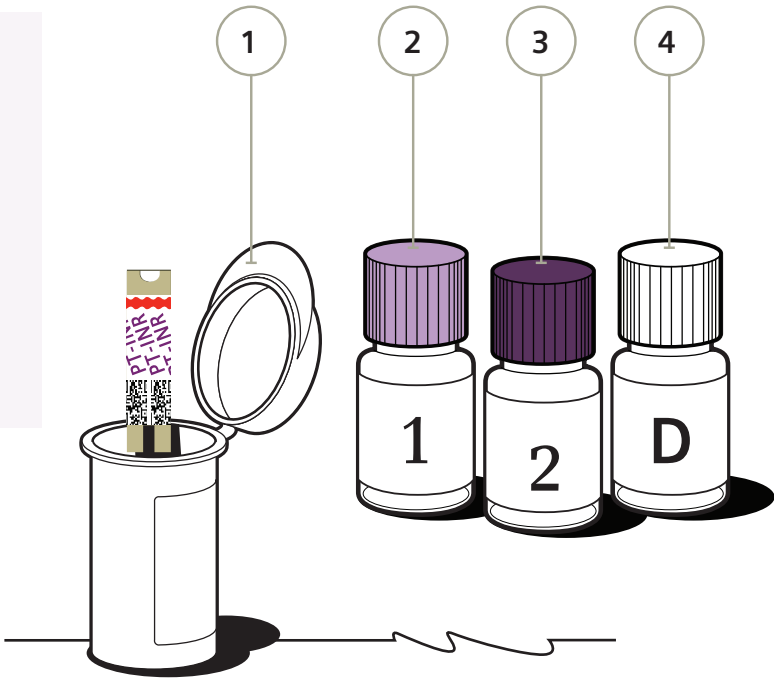


GETTING STARTED

- 1 Install batteries.

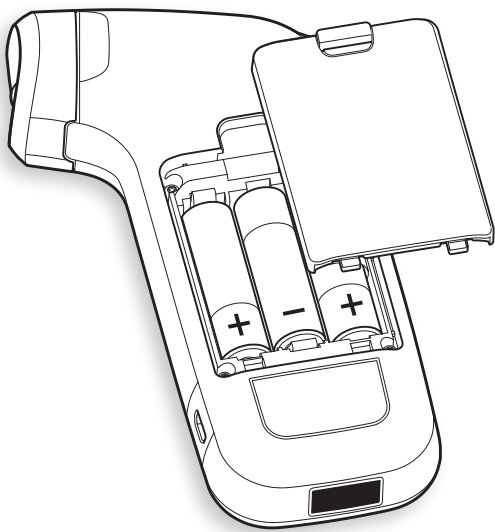


- 2 Turn Stride on by pressing the On/Off button.

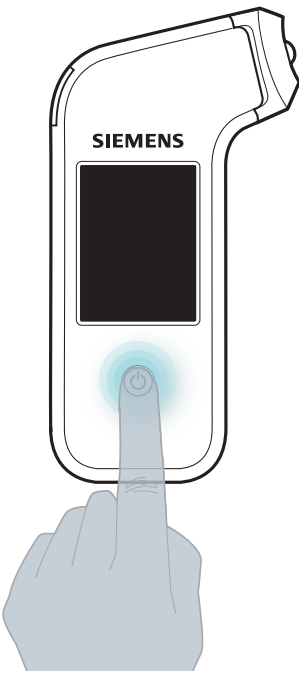



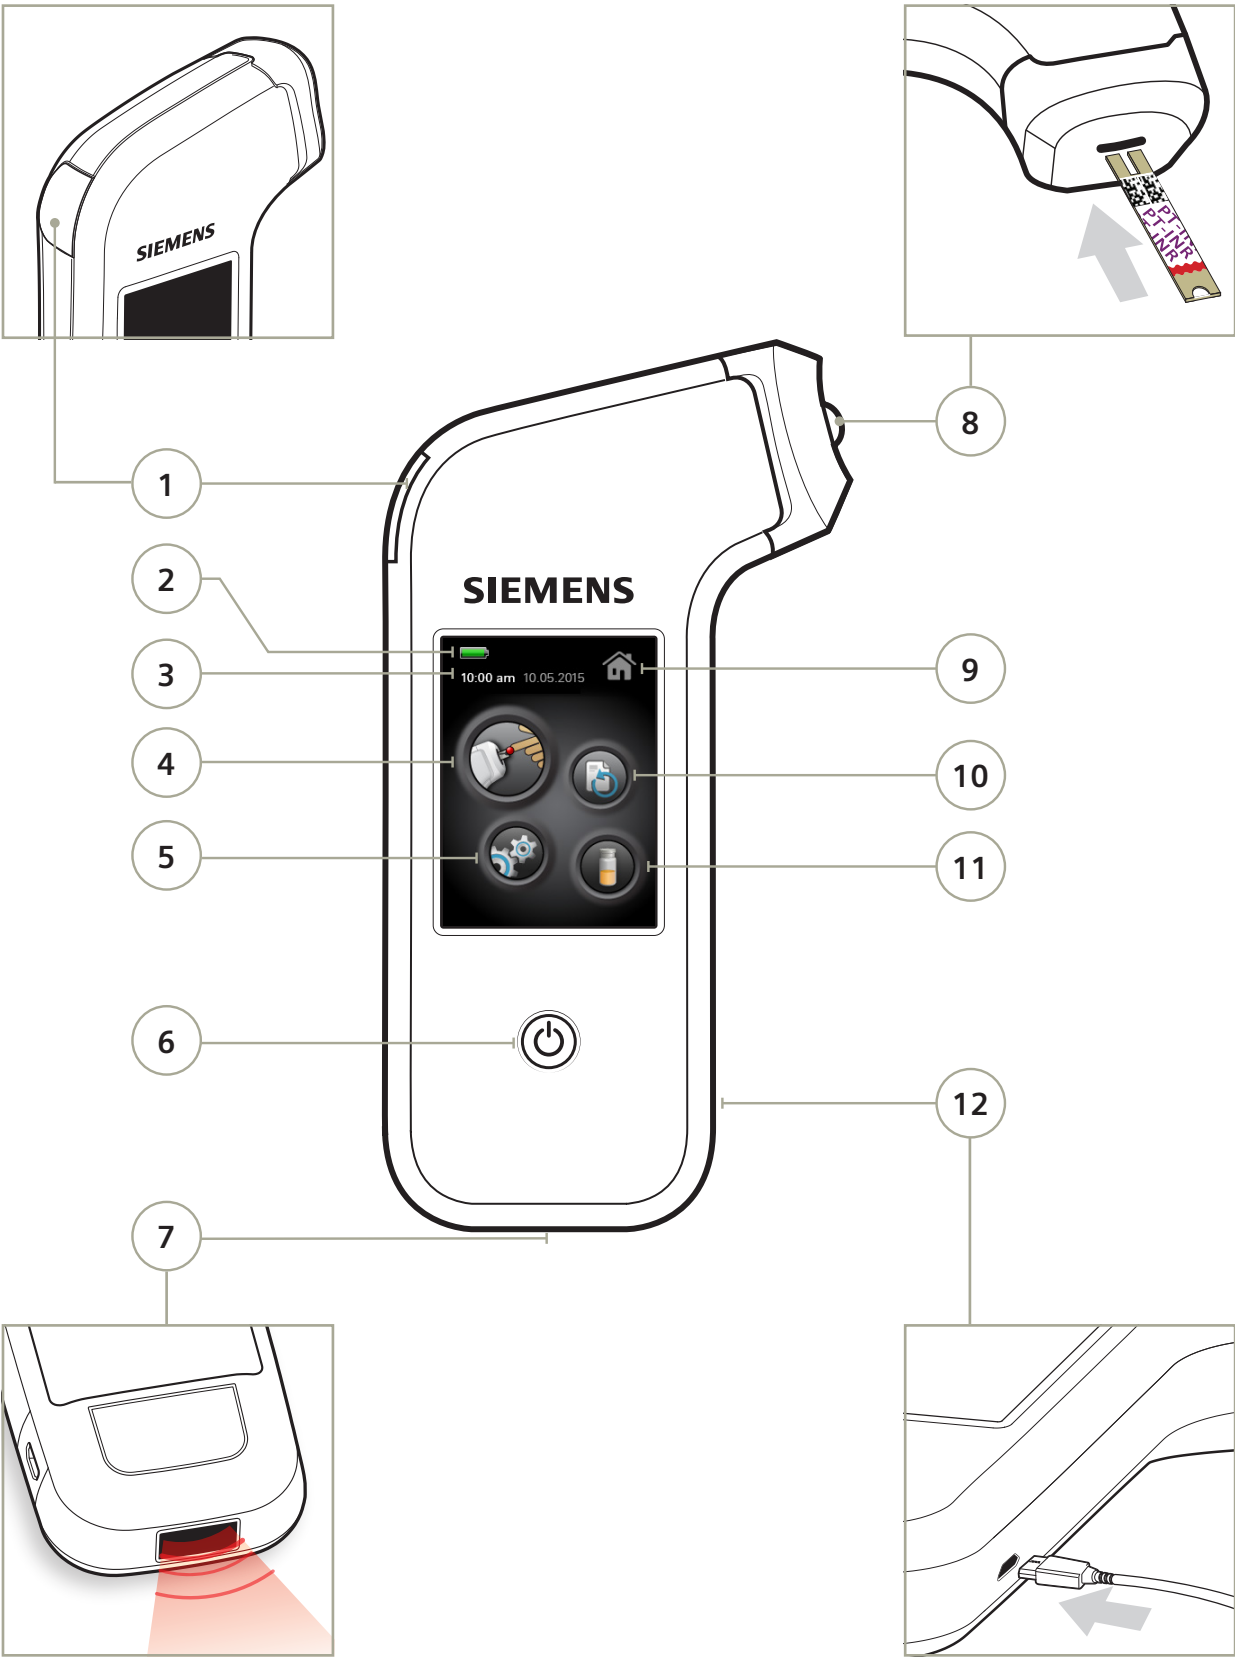




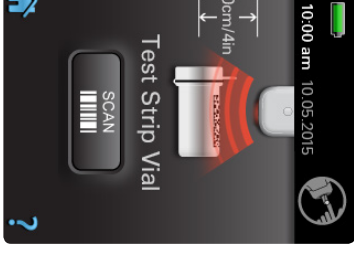
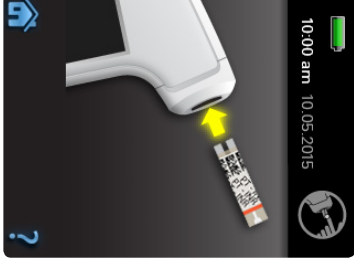
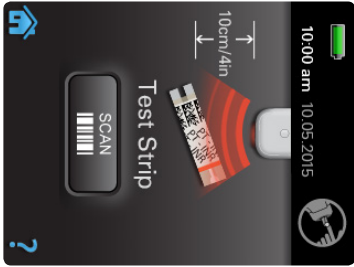


ANALYZER OVERVIEW

- 1 Test Strip Eject Button
- 2 Battery Power
- 3 Time and Date
- 4 Patient Test
- 5 Settings
- 6 On/Off Button
- 7 Barcode Reader
- 8 Test Strip Port
- 9 Current Screen
- 10 Recall Results
- 11 Quality Control Test
- 12 USB Connection

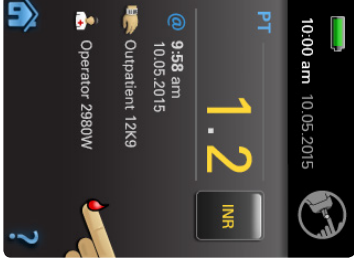

► This document is designed as a reference to be used alongside the Xprecia Stride Coagulation Analyzer. For complete instructions, see the *Xprecia Stride User Guide* and the instructions for use that came with your test strips and controls.

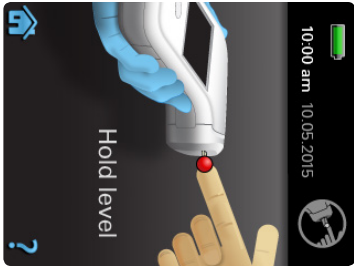Patient Test



1 Scan Patient ID (optional).

2 Scan strip.

3 Insert strip.

4 Scan strip vial (optional).

5 Prepare sample.

6 Hold level.

7 Apply sample.


8 Test in progress.

9 View result.


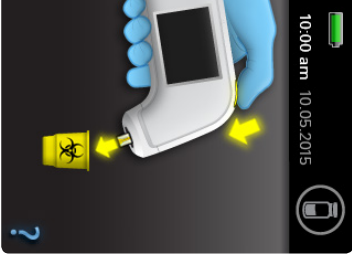
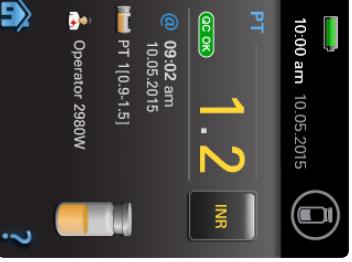

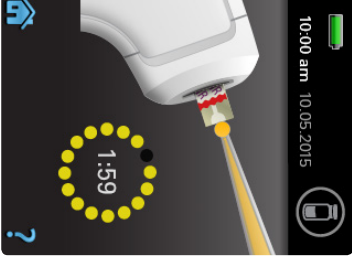



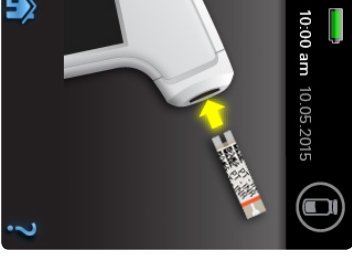

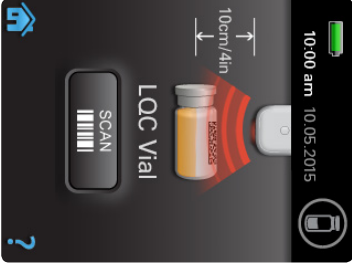

10 Eject strip.

11 Clean Stride.

Quality Control Test



IMPORTANT ► Prepare Xprecia Systems PT Controls in advance and allow to stand for 5 minutes. Use the reconstituted control solution within 25 minutes, when stored at 15–25°C (59–77°F). For complete instructions, see the *Xprecia Stride User Guide* and the instructions for use that came with your controls.



1 Scan control solution bottle.

2 Scan strip.

3 Insert strip.

4 Scan strip vial (optional).

5 Gather controls.

6 Hold level.

7 Apply control sample.

8 Test in progress.


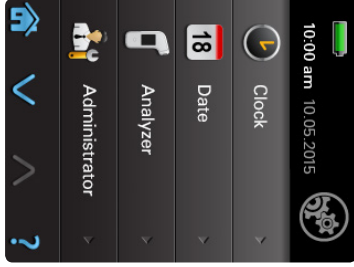

9 View result.

10 Eject strip.

11 Clean Stride.

REFERENCE INFORMATION

Settings






1 Clock

2 Date

3 Analyzer

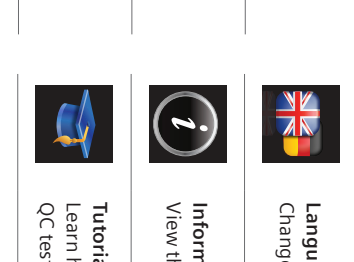4 Administrator






1 Clock

2 Date

3 Analyzer

4 Administrator

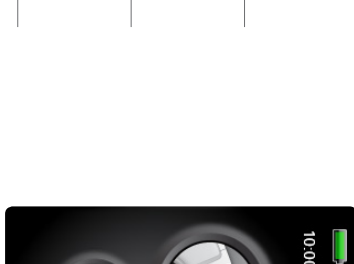
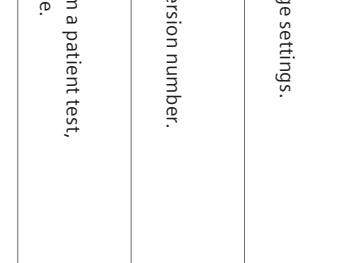
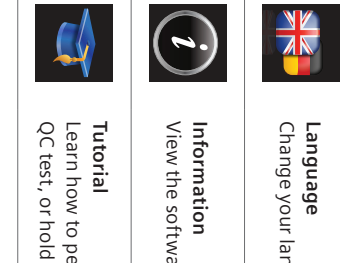



1 Language

2 Information

3 Tutorial

Recall Results

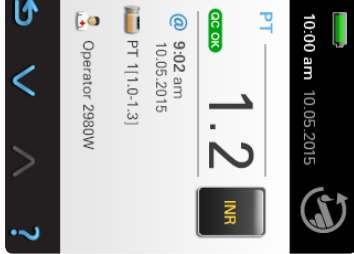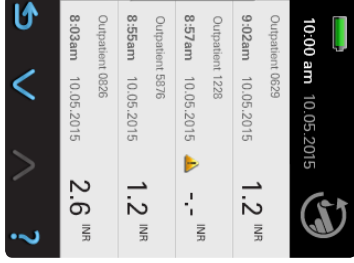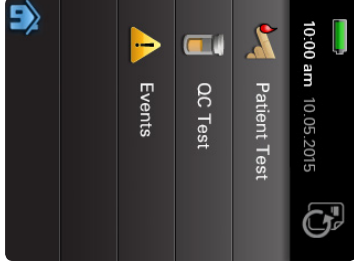

1 Tap a result type.

2 Tap a result to view details.

3 Tap ✓ to view more details.

For complete cleaning instructions, see the *Xprecia Stride User Guide*.